


1282-1  
NOSY

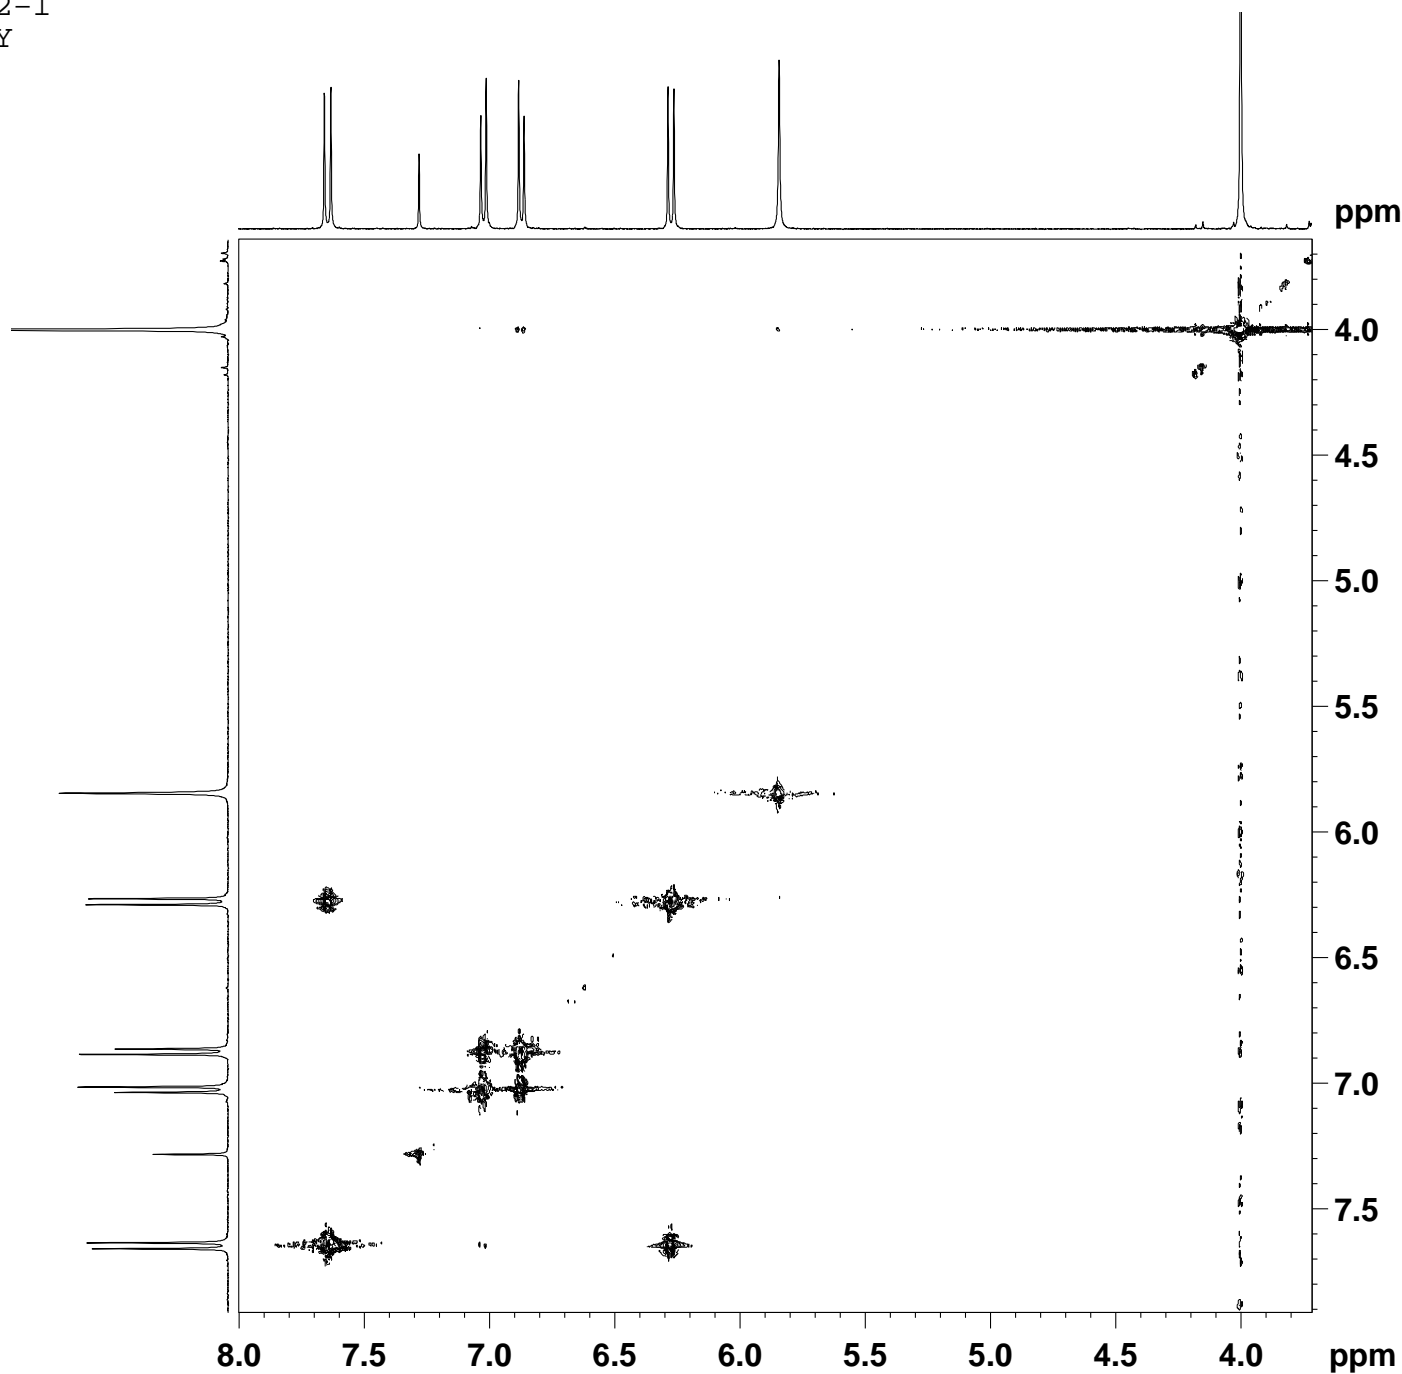

Current Data Parameters  
NAME 1282-1  
EXPNO 2  
PROCNO 2  
DU /m  
USER quamar

F2 - Acquisition Parameters  
Date\_ 20110111  
Time 12.41  
INSTRUM DPX400  
PROBHD 5 mm BBO BB-1H  
PULPROG noesygpph  
TD 2048  
SOLVENT CDCl3  
NS 2  
DS 1  
SWH 3205.128 Hz  
FIDRES 1.565004 Hz  
AQ 0.3195380 sec  
RG 322.5  
DW 156.000 usec  
DE 6.00 usec  
TE 298.2 K  
d0 0.00013896 sec  
D1 2.00000000 sec  
D8 0.40000001 sec  
D16 0.00025000 sec  
IN0 0.00031230 sec  
TAU 0.19875000 sec

==== CHANNEL f1 =====  
NUC1 1H  
P1 13.50 usec  
P2 27.00 usec  
PL1 -3.00 dB  
SFO1 400.2466000 MHz

==== GRADIENT CHANNEL =====  
GPNAM1 SINE.100  
GPNAM2 SINE.100  
GPZ1 40.00 %  
GPZ2 -40.00 %  
P16 1000.00 usec

F1 - Acquisition parameters  
ND0 1  
TD 256  
SFO1 400.2466 MHz  
FIDRES 12.508005 Hz  
SW 8.000 ppm  
FnMODE TPPI

F2 - Processing parameters  
SI 2048  
SF 400.2450000 MHz  
WDW EM  
SSB 0  
LB 2.00 Hz  
GB 0  
PC 1.40

F1 - Processing parameters  
SI 2048  
MC2 TPPI  
SF 400.2450000 MHz  
WDW QSINE  
SSB 2  
LB 0.00 Hz  
GB 0