

Sample #11 COSY



Current Data Parameters
NAME sample11
EXPNO 5
PROCNO 1

F2 - Acquisition Parameters
Date_ 20001218
Time 12.34
INSTRUM dpx400
PROBHD 5 mm BBO Z-Gra
PULPROG cosygp
TD 1024
SOLVENT CDCL3
NS 2
DS 4
SWH 400.641 Hz
FIDRES 0.391251 Hz
AQ 1.2779520 sec
RG 57
DW 1248.000 usec
DE 6.00 usec
TE 300.0 K
D0 0 sec
D1 1.50000000 sec
D13 0 sec
D16 0.00025000 sec
IN0 0.00249918 sec


===== CHANNEL f1 =====
NUC1 1H
P0 8.00 usec
P1 8.00 usec
PL1 -3.00 dB
SFO1 400.1328009 MHz

===== GRADIENT CHANNEL =====
GPNAM[1] SINE.100
GPNAM[2] SINE.100
GPX1 0 %
GPX2 0 %
GPY1 0 %
GPY2 0 %
GPZ1 10.00 %
GPZ2 10.00 %
P16 1000.00 usec

F1 - Acquisition parameters
TD 128
SFO1 400.1328 MHz
FIDRES 6.252063 Hz
SW 1.000 ppm
FnMODE undefined

F2 - Processing parameters
SI 2048
SF 400.1300094 MHz
WDW SINE
SSB 0
LB 0 Hz
GB 0
PC 1.40

F1 - Processing parameters
SI 1024
MC2 QF
SF 400.1300094 MHz
WDW SINE
SSB 0
LB 0 Hz
GB 0

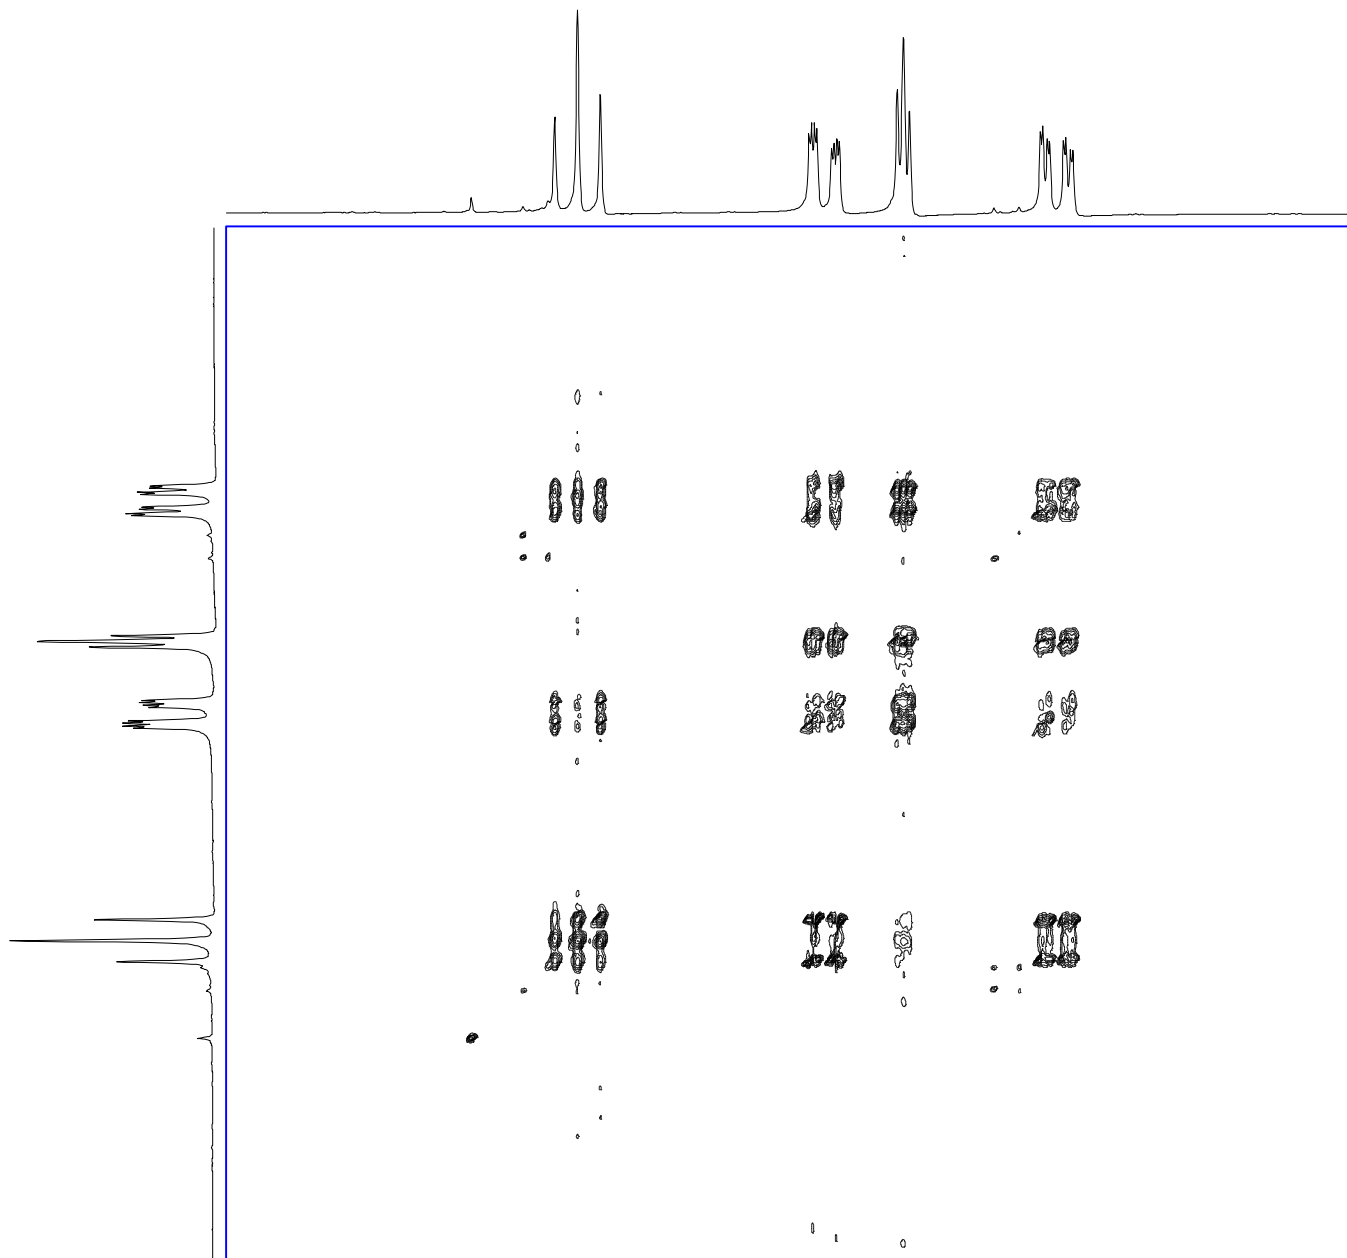

7.4 7.3 7.2 7.1 7.0 6.9 6.8 6.7 6.6 6.5 ppm

ppm
6.5
6.6
6.7
6.8
6.9
7.0
7.1
7.2
7.3
7.4