


Sample #36

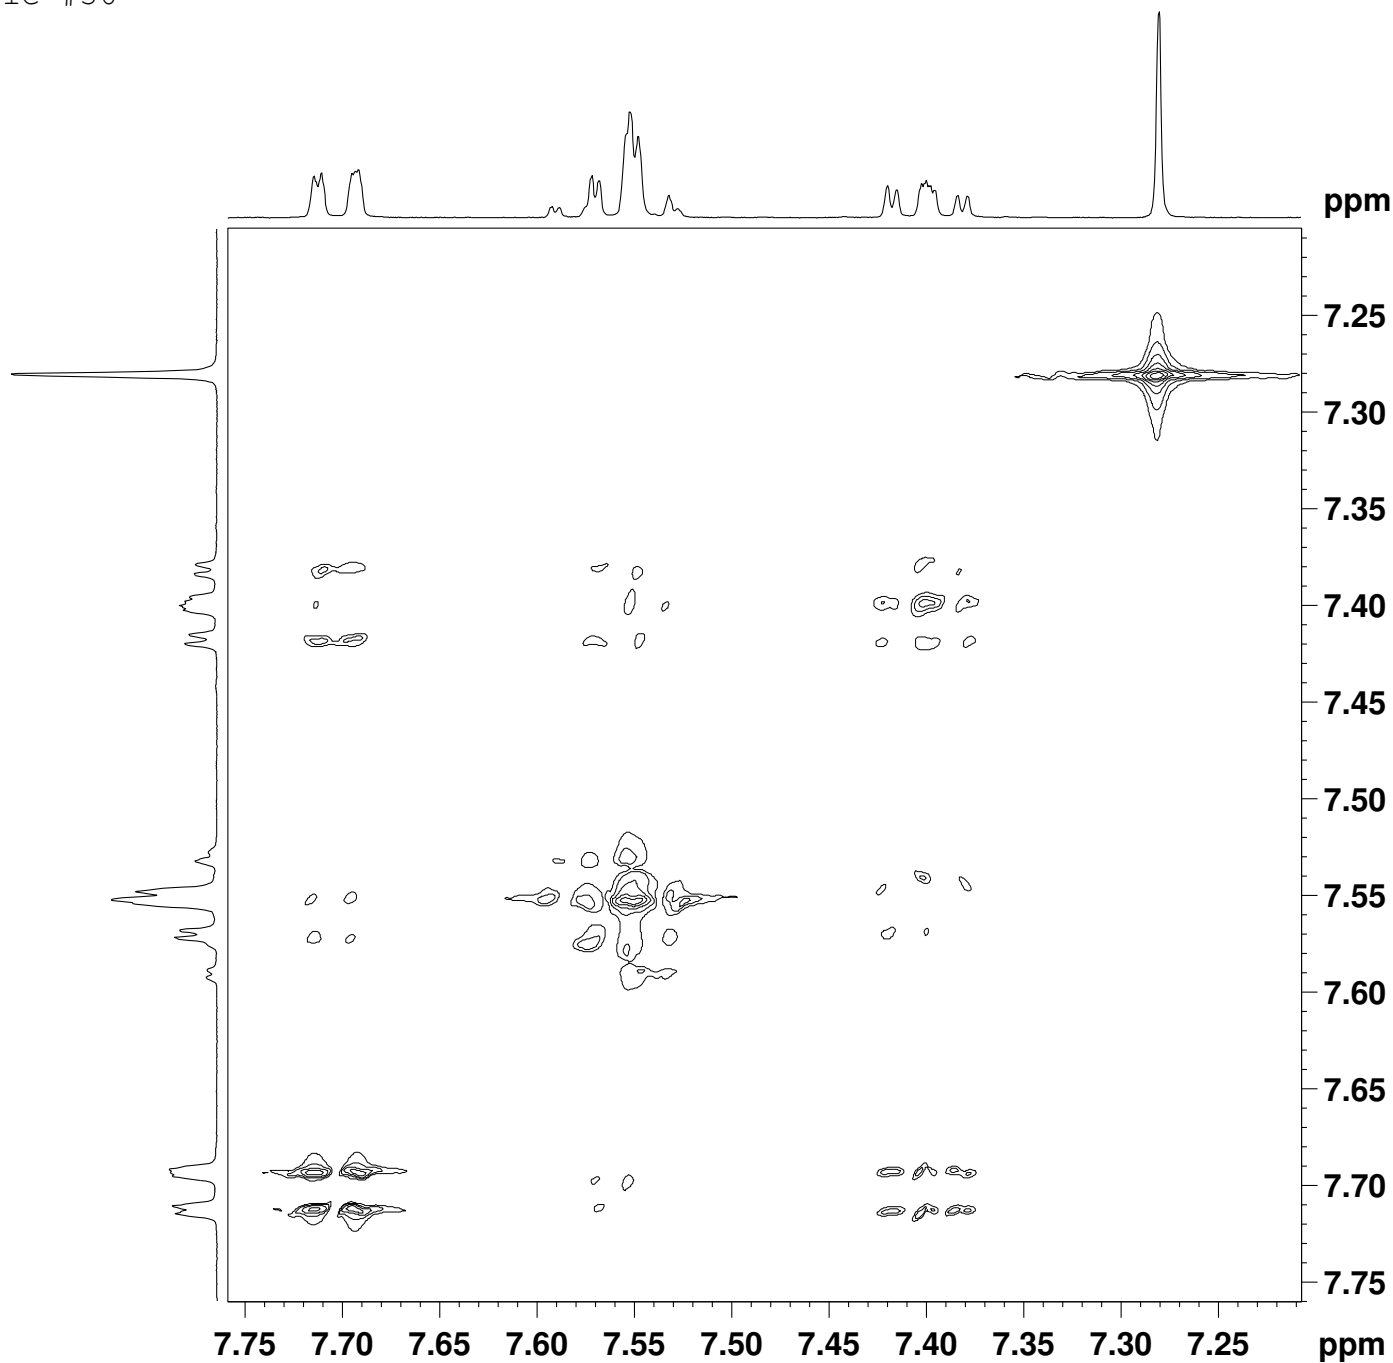

NAME Un\_36  
EXPNO 3  
PROCNO 1  
Date\_ 20110426  
Time 14.16  
INSTRUM DPX400  
PROBHD 5 mm BBO BB-1H  
PULPROG cosygpgf  
TD 1024  
SOLVENT CDC13  
NS 2  
DS 4  
SWH 801.282 Hz  
FIDRES 0.782502 Hz  
AQ 0.6390260 sec  
RG 3649.1  
DW 624.000 usec  
DE 6.00 usec  
TE 298.2 K  
d0 0.00000300 sec  
D1 2.00000000 sec  
d13 0.00000400 sec  
D16 0.00025000 sec  
IN0 0.00124800 sec

==== CHANNEL f1 =====  
NUC1 1H  
P0 13.50 usec  
P1 13.50 usec  
PL1 -3.00 dB  
SFO1 400.2480018 MHz

==== GRADIENT CHANNEL =====  
GPNAM1 SINE.100  
GPNAM2 SINE.100  
GPZ1 10.00 %  
GPZ2 10.00 %  
P16 1000.00 usec  
ND0 1  
TD 128  
SFO1 400.248 MHz  
FIDRES 6.260016 Hz  
SW 2.002 ppm  
FnMODE QF  
SI 2048  
SF 400.2450000 MHz  
WDW QSINE  
SSB 2  
LB 0.00 Hz  
GB 0  
PC 1.40  
SI 2048  
MC2 QF  
SF 400.2450000 MHz  
WDW QSINE  
SSB 2  
LB 0.00 Hz  
GB 0