


Unknown 45

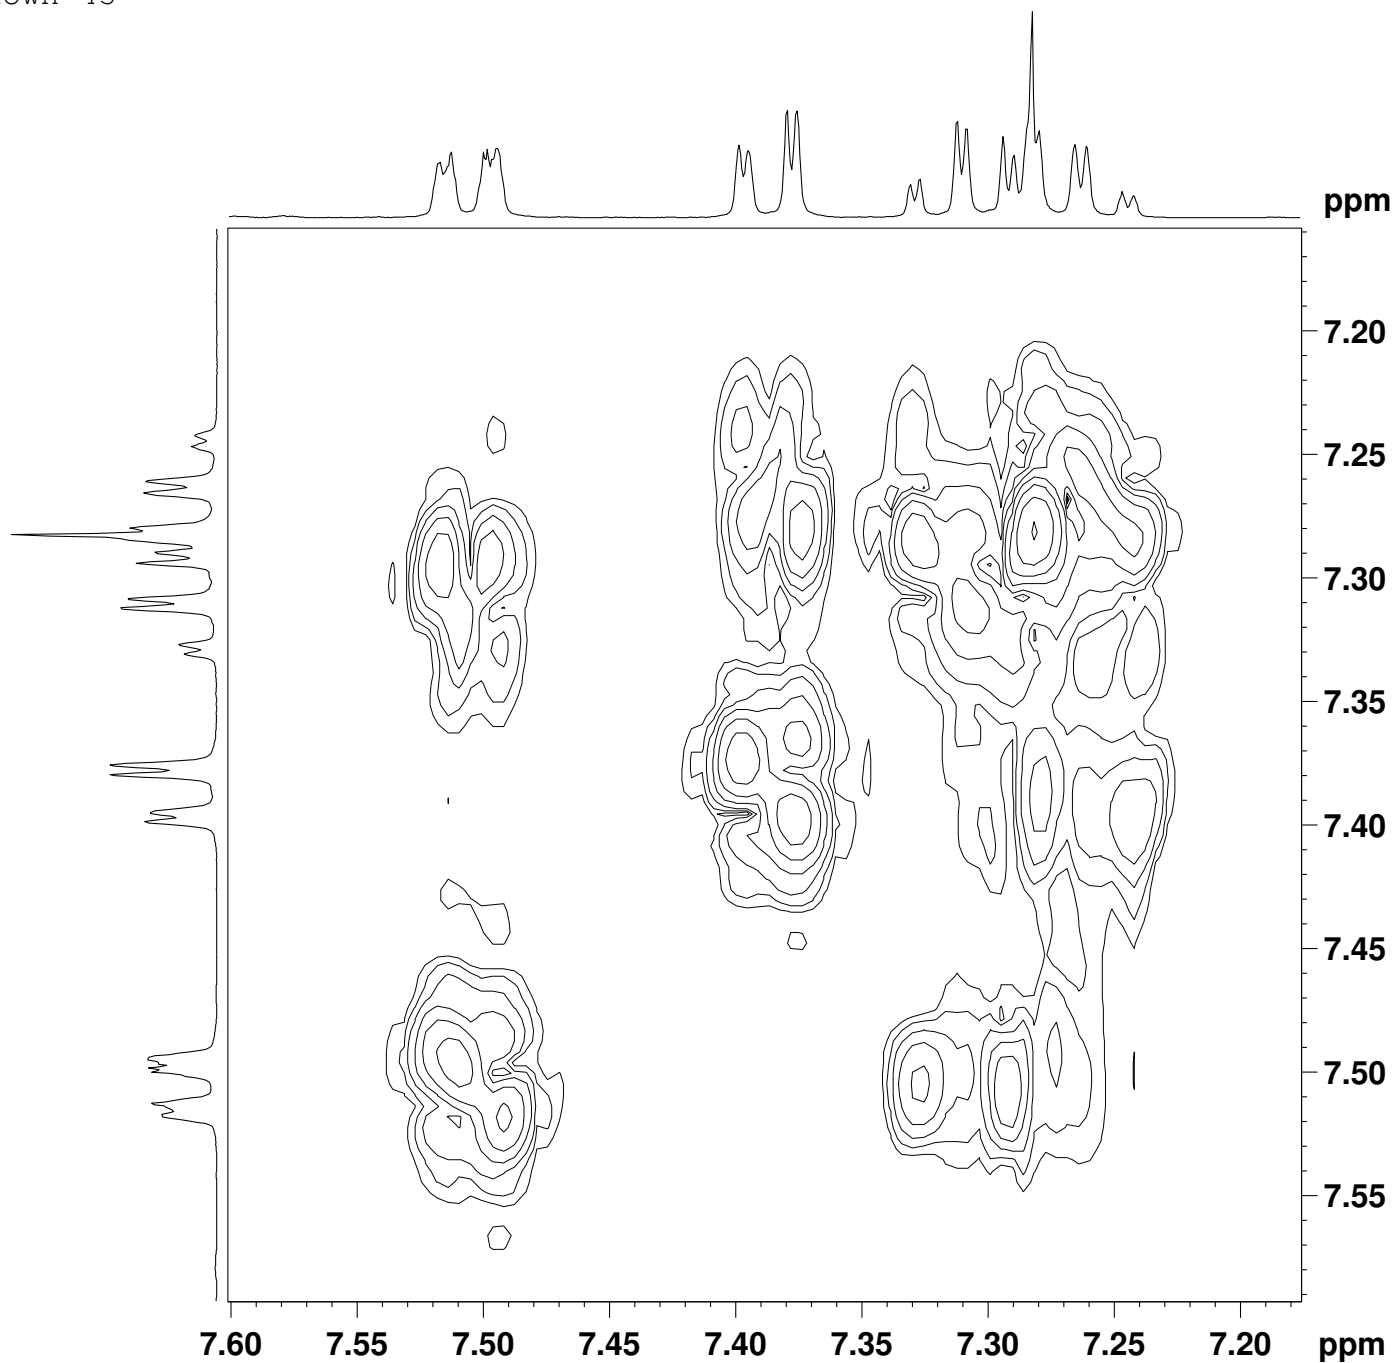

```
NAME           Un_45
EXPNO           3
PROCNO          1
Date_          20120222
Time            9.00
INSTRUM        robinson
PROBHD         5 mm PABBO BB-
PULPROG        cosygpgqf
TD             2048
SOLVENT        CDC13
NS              2
DS              8
SWH            3591.954 Hz
FIDRES         1.753884 Hz
AQ             0.2851316 sec
RG             574.7
DW             139.200 usec
DE             6.50 usec
TE             298.2 K
D0             0.00000300 sec
D1             2.00000000 sec
D13            0.00000400 sec
D16            0.00020000 sec
IN0            0.00027840 sec
```

```
===== CHANNEL f1 =====
NUC1            1H
P0              14.00 usec
P1              14.00 usec
PL1             0.00 dB
SFO1            400.1418006 MHz
```

```
===== GRADIENT CHANNEL =====
GPNAM1         SINE.100
GPZ1           10.00 %
P16            1000.00 usec
ND0            1
TD             256
SFO1            400.1418 MHz
FIDRES         14.031069 Hz
SW             8.977 ppm
FnMODE         QF
SI             2048
SF             400.1400000 MHz
WDW            SINE
SSB            0
LB             0.00 Hz
GB            0
PC             1.40
SI             2048
MC2           QF
SF             400.1400000 MHz
WDW            SINE
SSB            0
LB             0.00 Hz
GB            0
```