


Unknown 47

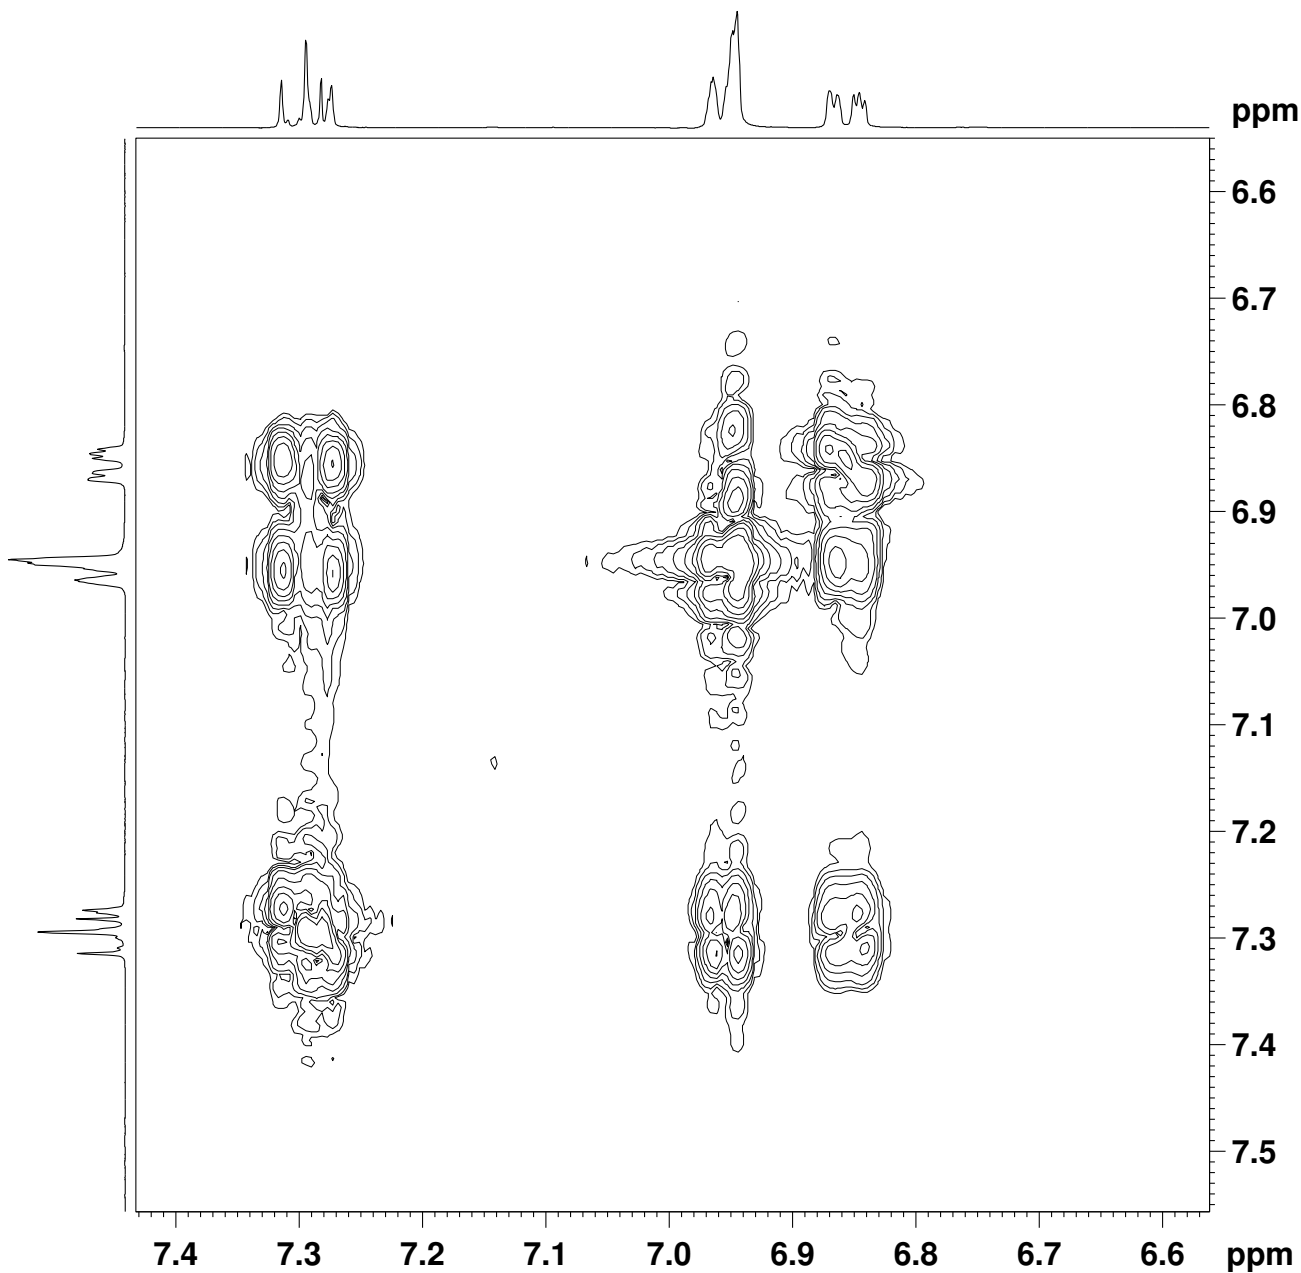

```
NAME          Un_47
EXPNO         3
PROCNO        1
Date_         20120222
Time          15.44
INSTRUM       robinson
PROBHD        5 mm PABBO BB-
PULPROG       cosygpgf
TD            2048
SOLVENT       CDC13
NS            2
DS            8
SWH           3591.954 Hz
FIDRES        1.753884 Hz
AQ            0.2851316 sec
RG            128
DW            139.200 usec
DE            6.50 usec
TE            298.2 K
D0            0.00000300 sec
D1            2.00000000 sec
D13           0.00000400 sec
D16           0.00020000 sec
IN0           0.00027840 sec
```

```
===== CHANNEL f1 =====
NUC1          1H
P0            14.00 usec
P1            14.00 usec
PL1           0.00 dB
SFO1          400.1418006 MHz
```

```
===== GRADIENT CHANNEL =====
GPNAM1        SINE.100
GPZ1          10.00 %
P16           1000.00 usec
ND0           1
TD            256
SFO1          400.1418 MHz
FIDRES        14.031069 Hz
SW            8.977 ppm
FnMODE        QF
SI            2048
SF            400.1400000 MHz
WDW           SINE
SSB           0
LB            0.00 Hz
GB            0
PC            1.40
SI            2048
MC2          QF
SF            400.1400000 MHz
WDW           SINE
SSB           0
LB            0.00 Hz
GB            0
```